


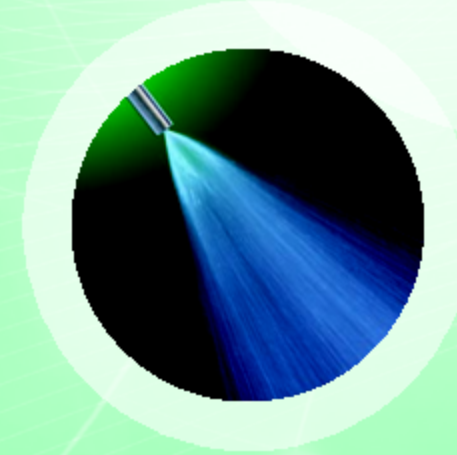


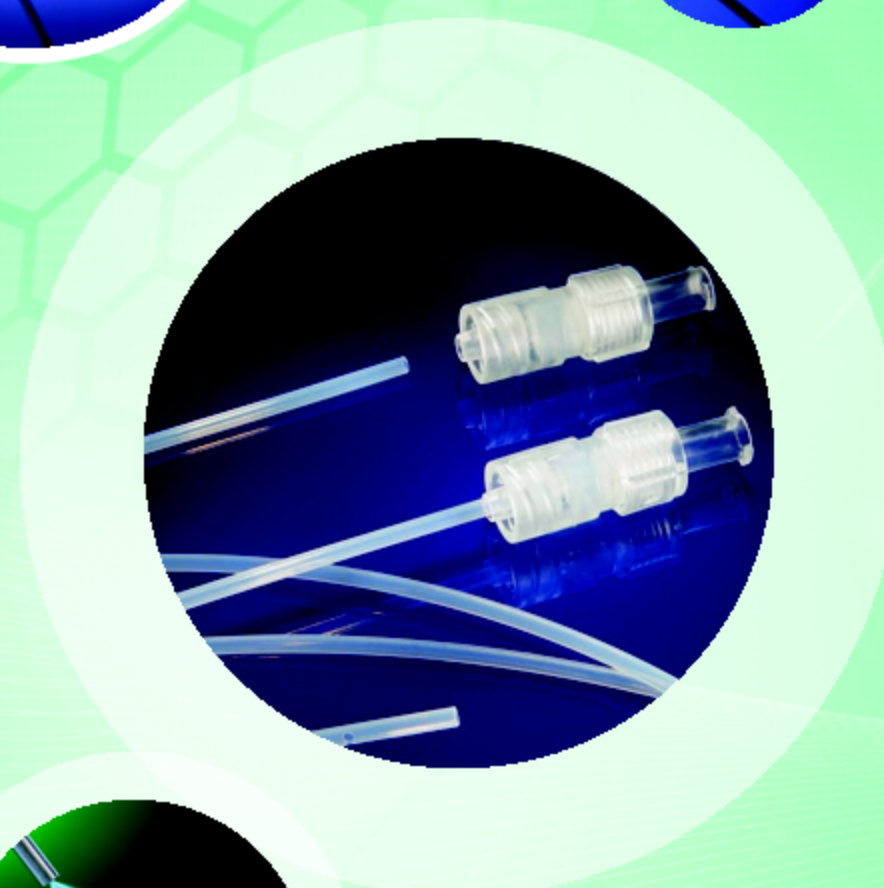

8 SPRING STREET, STAFFORD SPRINGS, CT 06076 • 800 344 6227 • WWW.HOBBSMEDICAL.COM



HOBBS MEDICAL, INC.



## INTRODUCTION

### WELCOME

Established in 1984, Hobbs Medical, Inc.

has built a solid reputation for

innovation and quality. A privately

held company with expertise in the

development and manufacture of

diagnostic and therapeutic accessories for

flexible GI and Pulmonary Endoscopy, Hobbs

works with a network of industry professionals,

consultants, sales representatives and international distribution agencies

to bring precision endoscopic accessories to the world market. We take pride in

our comprehensive line of precision accessories, all manufactured in the USA, and

continue to introduce unique devices to the ever-changing market.

The entire staff at Hobbs Medical is committed to exceeding each and every customer's expectations;

providing cost-effective, quality and innovative products and investing in ongoing product development.

Our Sales personnel are always available to answer inquiries. We look forward to responding to your needs.

Contact Sales at (800) 344-6227 or visit [www.hobbsmedical.com](http://www.hobbsmedical.com)



**HOBBS MEDICAL, INC.** 8 SPRING STREET, STAFFORD SPRINGS, CT 06076 • 800 344 6227 • [WWW.HOBBSMEDICAL.COM](http://WWW.HOBBSMEDICAL.COM)

**ALL HOBBS MEDICAL PRODUCTS ARE PROUDLY MANUFACTURED IN THE USA.  
HOBBS MEDICAL IS ISO-13485 REGISTERED; CE-CERTIFIED AND COMPLIES WITH  
COUNCIL DIRECTIVE 93/94EEC AND FDA QUALITY SYSTEMS REGULATIONS.**

**Customer Service**  
800-344-6227 toll-free  
860-684-5875  
860-684-7574 fax  
[customerservice@hobbsmedical.com](mailto:customerservice@hobbsmedical.com)

**Sales**  
800-344-6227 toll-free  
860-684-5875  
[salesdept@hobbsmedical.com](mailto:salesdept@hobbsmedical.com)

## QUALITY POLICY

The Quality Policy of Hobbs Medical, Inc. is to meet the needs and expectations of our customers. This will be accomplished through market feedback and continuous evaluation of our Quality Management System to ensure its continued effectiveness and suitability in complying with customer needs and all regulatory requirements at all levels of the organization.

## SPECIFICATION CHANGES

Hobbs Medical reserves the right to make improvements and changes in the products described herein. Should you have a suggestion for a new device or an improvement of an existing device, let our Engineering staff translate your idea into reality. Our website ([www.hobbsmedical.com](http://www.hobbsmedical.com)) provides an avenue for product suggestions.

## PRODUCT WARRANTY

Descriptions or specifications appearing in Hobbs Medical literature are solely meant to generally describe the product at the time of manufacture and do not constitute any express warranties. Hobbs Medical warrants all of its products to be free from defects in materials and workmanship. Storage conditions and product use are factors beyond the control of Hobbs Medical and may directly affect the products and the results obtained from them. The user assumes responsibility for any consequences, which may arise from the final use of the products. No person has any authority to bind Hobbs Medical to any representation or warranty concerning these products.

All reusable products in this catalog are warranted to the original purchaser to be free from defects in material and workmanship for a period of six months from the date of purchase. All disposable products are warranted to the original purchaser to be free from defects in materials and workmanship for the first use only.

## RETURN POLICY

A Return Authorization Number must be obtained for all returned products. Contact our Customer Service Department (800-344-6227). Returns must include a reason for return, lot number, catalog number and invoice number. Contaminated products sent for evaluation will not be accepted unless the product has been cleaned and high level disinfected prior to returning to Hobbs Medical. Returned, unused products must be in the original unopened Hobbs Medical pouch and will be subject to a 20% restocking fee.

## SHIPPING & TERMS

Most items are shipped within one day. Products are shipped via ground transportation unless otherwise specified. MasterCard and VISA accepted. F.O.B. Stafford Springs, Connecticut. Due to fluctuating operating costs, we reserve the right to change prices without prior notice.

## ORDERING INFORMATION

Our Sales and Customer Service personnel are always available to answer inquiries and to meet our customers' specific needs. Order and Price Requests can be placed by telephone, fax or email.

## CONTACT INFORMATION

**Customer Service**  
**800-344-6227 toll-free**  
**860-684-5875**  
**860-684-7574 fax**  
**[customerservice@hobbsmedical.com](mailto:customerservice@hobbsmedical.com)**

**Sales**  
**800-344-6227 toll-free**  
**860-684-5875**  
**[salesdept@hobbsmedical.com](mailto:salesdept@hobbsmedical.com)**

*Orders & Returns*

*Product Information*  
*Pricing*  
*Specification Changes*


# BALLOONS

BALLOONS

## GASTROINTESTINAL PRODUCTS

### Achalasia Balloon Dilators

- Guide Wire port accepts a .038 inch Guide Wire
- Standard Luer-lock fittings for compatibility with inflation/deflation devices
- Radiopaque markers located within the balloon aids in the positioning of the balloon under fluoroscopy
- Multiple diameters offered
- No minimum order requirements
- Packaged sterile for single use

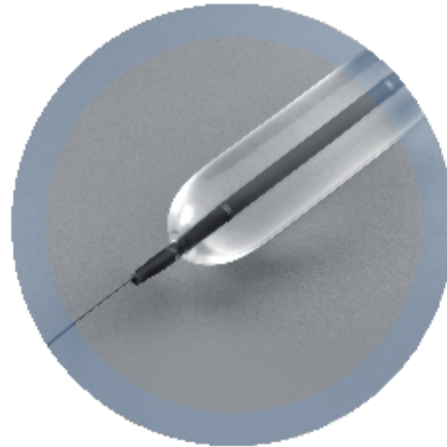

#### ACHALASIA BALLOON DILATORS

Catalog Number	Description	Inflated O.D.	Balloon Length	Sheath	Length
3302	Over the Wire	30mm (90fr)	10cm	5.3mm	100cm
3304	Over the Wire	35mm (105fr)	10cm	5.3mm	100cm
3306	Over the Wire	40mm (120fr)	10cm	5.3mm	100cm

#### ACHALASIA BALLOON DILATOR KIT

Catalog Number	Kit Includes	Inflated O.D.
3300	3302	30mm (90fr)
	3204	35mm (105fr)
	3306	40mm (120fr)
	3406 Guide Wire	




**HOBBS MEDICAL, INC.**

8 SPRING STREET, STAFFORD SPRINGS, CT 06076 • 800 344 6227 • WWW.HOBBSMEDICAL.COM

## GASTROINTESTINAL PRODUCTS

### Biliary Balloon Dilators

- Offered in a range of inflated diameters and balloon lengths
- Accepts a .035 inch Guide Wire
- Radiopaque markers for easy visibility under fluoroscopy
- No minimum order requirements
- Packaged sterile for single use

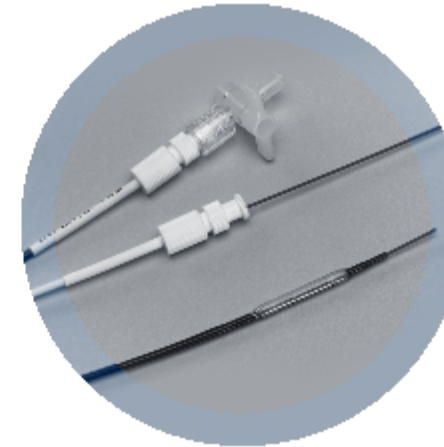

#### BILIARY BALLOON DILATORS

Catalog Number	Description	Inflated O.D.	Balloon Length	Sheath	Length	Working Channel
3180	Over the Wire	4mm (12fr)	2cm	2.3mm	180cm	2.8mm
3182	Over the Wire	6mm (18fr)	2cm	2.3mm	180cm	2.8mm
3184	Over the Wire	8mm (24fr)	3cm	2.3mm	180cm	2.8mm

#### BILIARY BALLOON DILATOR KIT

Catalog Number	Kit Includes	Balloon O.D.
3006	3180	4mm (12fr)
	3182	6mm (18fr)
	3184	8mm (24fr)
	3412 Guide Wire	



**HOBBS MEDICAL, INC.**


8 SPRING STREET, STAFFORD SPRINGS, CT 06076 • 800 344 6227 • WWW.HOBBSMEDICAL.COM



## GASTROINTESTINAL PRODUCTS

### Stone Extraction (OTW) Balloons

- Accepts a .035 inch Guide Wire
- Balloon material is compatible with ERCP solutions
- Range of inflated diameters to meet your procedural needs
- Unique shape prevents balloon from slipping past stone during retraction
- Radiopaque markers for easy visibility under fluoroscopy
- Standard Luer-lock fitting on injection port
- No minimum order requirements
- Packaged sterile for single use

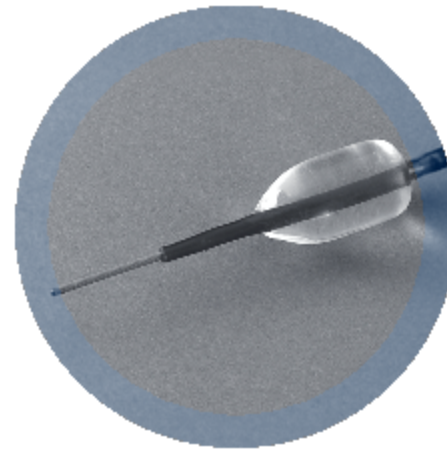

#### STONE EXTRACTION (OTW) BALLOONS

Catalog Number	Description	Inflated O.D.	Sheath	Length	Working Channel
3502	Over the Wire	10mm (30fr)	2.3mm	180cm	2.8mm
3503	Over the Wire	13mm (39fr)	2.3mm	180cm	4.2mm
3504	Over the Wire	16mm (48fr)	2.3mm	180cm	4.2mm

#### INFLATION-DEFLATION SYSTEM


Catalog Number	Description
3900	Vacu-lok Aspirating Syringe
4630	Inflation Monitor



## GASTROINTESTINAL PRODUCTS

### Flex-Ez Guide Wires

- Provides a cost-effective alternative when a generic Guide Wire is required to assist in placing Esophageal Stents, Over the Wire Balloon Dilators or Achalasia Balloons
- Teflon coating provides easy passage through the endoscope's working channel
- Packaged sterile for single use

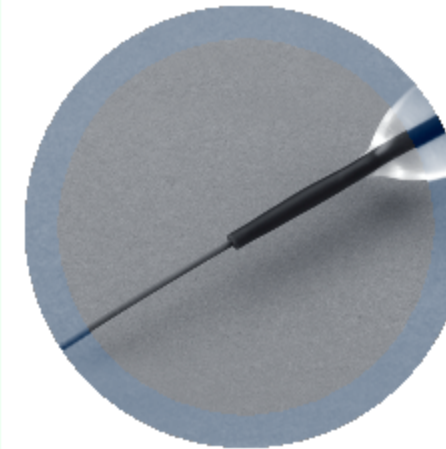

#### FLEX-EZ GUIDE WIRES


Catalog Number	Description	O.D.	Style	Length
3406	Floppy Tip	.038in	Teflon Coated	260cm
3410	Floppy Tip	.035in	Teflon Coated	260cm
3412	Floppy Tip	.035in	Teflon Coated	400cm



## GASTROINTESTINAL PRODUCTS

### Flex-Ez Over the Wire (OTW) Balloon Dilators

- Designed to meet Esophageal, Pyloric and Colonic dilation requirements
- Complete range of balloon lengths (3cm, 4cm and 8cm) and inflated diameters (6mm to 20mm)
- Accepts a .035 inch Guide Wire
- Radiopaque markers for easy visibility under fluoroscopy
- Uniform dilation performance under recommended gradual inflation pressure
- No minimum order requirements
- Packaged sterile for single use

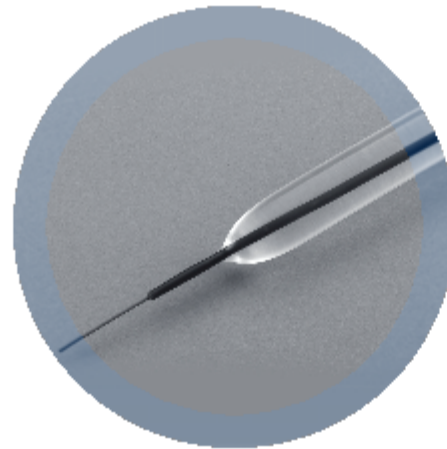

#### FLEX-EZ OVER THE WIRE (OTW) BALLOON DILATORS

Catalog Number	Description	Inflated O.D.	Balloon Length	Sheath	Length	Working Channel
3152	Over the Wire	8mm (24fr)	3cm	2.3mm	240cm	2.8mm
3156	Over the Wire	10mm (30fr)	3cm	2.3mm	240cm	2.8mm
3158	Over the Wire	12mm (36fr)	3cm	2.3mm	240cm	2.8mm
3206	Over the Wire	14mm (42fr)	3cm	2.3mm	240cm	3.7mm
3208	Over the Wire	16mm (48fr)	3cm	2.3mm	240cm	3.7mm
3210	Over the Wire	18mm (54fr)	3cm	2.3mm	240cm	3.7mm
3212	Over the Wire	20mm (60fr)	3cm	2.3mm	240cm	3.7mm
3102	Over the Wire	6mm (18fr)	4cm	2.3mm	240cm	2.8mm
3104	Over the Wire	8mm (24fr)	4cm	2.3mm	240cm	2.8mm
3106	Over the Wire	10mm (30fr)	4cm	2.3mm	240cm	2.8mm
3202	Over the Wire	16mm (48fr)	4cm	2.3mm	240cm	3.7mm
3204	Over the Wire	20mm (60fr)	4cm	2.3mm	240cm	3.7mm
3250	Over the Wire	8mm (24fr)	8cm	2.3mm	240cm	3.7mm
3254	Over the Wire	10mm (30fr)	8cm	2.3mm	240cm	3.7mm
3258	Over the Wire	12mm (36fr)	8cm	2.3mm	240cm	3.7mm
3260	Over the Wire	14mm (42fr)	8cm	2.3mm	240cm	3.7mm
3262	Over the Wire	16mm (48fr)	8cm	2.3mm	240cm	3.7mm
3264	Over the Wire	18mm (54fr)	8cm	2.3mm	240cm	3.7mm
3266	Over the Wire	20mm (60fr)	8cm	2.3mm	240cm	3.7mm

#### FLEX-EZ GUIDE WIRE

Catalog Number	Description	O.D.	Style	Length
3412	Floppy Tip	.035in	Teflon Coated	400cm



## GASTROINTESTINAL PRODUCTS

#### FLEX-EZ OVER THE WIRE (OTW) BALLOON DILATOR KIT

Catalog Number	Kit Includes	Balloon O.D.	Balloon Length
3000	3102 Balloon	6mm (18fr)	4cm
	3104 Balloon	8mm (24fr)	4cm
	3106 Balloon	10mm (30fr)	4cm
	3250 Balloon	8mm (24fr)	8cm
	3254 Balloon	10mm (30fr)	8cm
	3258 Balloon	12mm (36fr)	8cm
	3260 Balloon	14mm (42fr)	8cm
	3262 Balloon	16mm (48fr)	8cm
	3264 Balloon	18mm (54fr)	8cm
	3266 Balloon	20mm (60fr)	8cm
	3412 Guide Wire		

#### INFLATION-DEFLATION SYSTEM

Catalog Number	Description
3900	Vacu-lok Aspirating Syringe
4630	Inflation Monitor



## GASTROINTESTINAL PRODUCTS

### Flex-Ez Stylet Wire Balloon Dilators

- Designed to meet all Esophageal, Pyloric and Colonic dilation requirements
- Complete range of balloon lengths (3cm, 5.5cm and 8cm) and inflated diameters (8mm to 20mm)
- Uniform dilation performance under recommended gradual inflation pressure
- No minimum order requirements
- Packaged sterile for single use



#### FLEX-EZ STYLET WIRE BALLOON DILATORS

Catalog Number	Description	Inflated O.D.	Balloon Length	Sheath	Length	Working Channel
3708	Stylet Wire	12mm (36fr)	8cm	2.3mm	240cm	2.8mm
3710	Stylet Wire	14mm (42fr)	8cm	2.3mm	240cm	2.8mm
3712	Stylet Wire	16mm (48fr)	8cm	2.3mm	240cm	2.8mm
3714	Stylet Wire	18mm (54fr)	8cm	2.3mm	240cm	2.8mm
3716	Stylet Wire	20mm (60fr)	8cm	2.3mm	240cm	2.8mm
3732	Stylet Wire	8mm (24fr)	5.5cm	2.3mm	240cm	2.8mm
3734	Stylet Wire	10mm (30fr)	5.5cm	2.3mm	240cm	2.8mm
3736	Stylet Wire	12mm (36fr)	5.5cm	2.3mm	240cm	2.8mm
3738	Stylet Wire	14mm (42fr)	5.5cm	2.3mm	240cm	2.8mm
3740	Stylet Wire	16mm (48fr)	5.5cm	2.3mm	240cm	2.8mm
3742	Stylet Wire	18mm (54fr)	5.5cm	2.3mm	240cm	2.8mm
3744	Stylet Wire	20mm (60fr)	5.5cm	2.3mm	240cm	2.8mm
3752	Stylet Wire	8mm (24fr)	3cm	2.3mm	240cm	2.8mm
3754	Stylet Wire	10mm (30fr)	3cm	2.3mm	240cm	2.8mm
3756	Stylet Wire	12mm (36fr)	3cm	2.3mm	240cm	2.8mm
3758	Stylet Wire	14mm (42fr)	3cm	2.3mm	240cm	2.8mm
3760	Stylet Wire	16mm (48fr)	3cm	2.3mm	240cm	2.8mm
3762	Stylet Wire	18mm (54fr)	3cm	2.3mm	240cm	2.8mm
3764	Stylet Wire	20mm (60fr)	3cm	2.3mm	240cm	2.8mm

#### FLEX-EZ STYLET WIRE BALLOON DILATOR KIT

Catalog Number	Kit Includes	Balloon O.D.	Balloon Length
3002	3708 Balloon	12mm (36fr)	8cm
	3710 Balloon	14mm (42fr)	8cm
	3712 Balloon	16mm (48fr)	8cm
	3714 Balloon	18mm (54fr)	8cm
	3716 Balloon	20mm (60fr)	8cm

#### INFLATION-DEFLATION SYSTEM

Catalog Number	Description
3900	Vacu-lok Aspirating Syringe
4630	Inflation Monitor



#### CONTACT INFORMATION

**Customer Service**  
**800-344-6227 toll-free**  
**860-684-5875**  
**860-684-7574 fax**  
**customerservice@hobbsmedical.com**

*Orders & Returns*

**Sales**  
**800-344-6227 toll-free**  
**860-684-5875**  
**salesdept@hobbsmedical.com**

*Product Information*  
*Pricing*  
*Specification Changes*